

Procedure for Nuts

See table below for consumable kit reorder number

- Use strips at room temperature 20–25 °C (68–77 °F).
- Bring the strip to room temperature if necessary.
- Do not open the strip pouch until ready to use the strip.

1

Calibrate the Vertu reader by scanning in the Afla-V AQUA barcode for the specific commodity and the lot of strips being used.



4

Transfer 100 µL of filtered extract to the Afla-V HS strip by dropping (~1 drop/second) vertically into the sample well. Allow the strip to develop for 5 minutes on a flat surface.



2

Weigh 10 g ± 0.1 g ground sample into extraction tube. Add 50 mL AQUA Premix to extraction tube.



5

Insert the Afla-V HS strip into the Vertu. Press the center key to take a reading. To print, use the arrow keys to move the cursor to "P" and press the center button.




3

Vortex at maximum speed for 2 minutes. Filter the extract into a clean tube for no more than 5 minutes.



6

To run the next sample, use the arrow keys to move the cursor to "NT" and press the center button on the keypad.

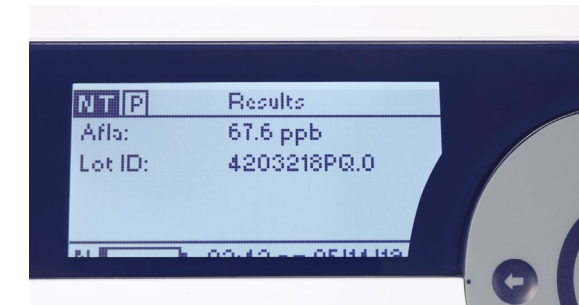

Strips should be stored at 2–30 °C (36–86 °F)
Store AQUA Premix at room temperature

Sample Type	Barcode*	Range/LOD	Reorder #
Peanuts	PQ	0–100 ppb/2 ppb	176004114PP
Peanut Paste	PPQ	0–80 ppb/1 ppb	176004114PP
Pecans	PC	0–50 ppb/2 ppb	176004114PC
Almonds	AQ	0–50 ppb/2 ppb	176004114AQ



Scan barcode to download the Strip Test Reference Guide

For additional information, please visit vicam.com/docs/vertu-strip-test-reference-guide



Orders:
Tel: +1-877.228.4244
+1-417.725.6588
Email: orders@vicam.com

Technical Support:
Tel: +1.800.338.4381
+1.508.482.4935
Email: techservice@vicam.com

715006792 Rev A IH

©2024 Waters Corporation. Waters, Afla-V, VICAM, and VERTU are trademarks of Waters Corporation.

WatersTM | VICAMTM

www.vicam.com