

Procedure for Grain

Consumable kit reorder number: 176002071VC

- Use strips at room temperature 20–25 °C (68–77 °F).
- Bring the strip to room temperature if necessary.

- Do not open the strip pouch until ready to use the strip.

1 Calibrate the Vertu reader by scanning in the Afla-V methanol barcode* and the lot of strips being used.




2 Weigh 5 g ± 0.1 g ground sample into extraction tube. Add 25 mL 70% MeOH to extraction tube.



3 Vortex at maximum speed for 2 minutes. Filter the extract into a clean tube for no more than 5 minutes.



4 Transfer 100 µL of the Afla-V diluent to a strip test vial. Add 100 µL of the filtered extract to the vial, cover and mix well by vortexing.

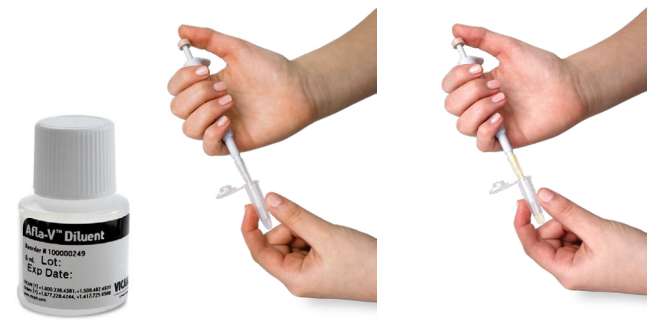

Strips must be stored at 2–30 °C (36–86 °F)

Store 70% MeOH at room temperature

*For corn and soy

Limit of Detection: 2 ppb


Range: 0–40 ppb (1st strip),
40–100 ppb (2nd strip with dilution)



Scan barcode to download the Strip Test Reference Guide
For additional information, please visit
vicam.com/docs/vertu-strip-test-reference-guide



5 Transfer 100 µL of filtered extract to the Afla-V strip by dropping (~1 drop/second) vertically into the sample well. Allow the strip to develop for exactly 5 minutes on a flat surface.

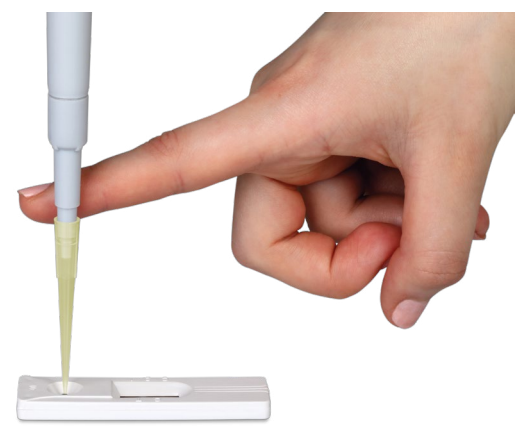

6 Insert the Afla-V strip into the Vertu. Press the center key to take a reading. To print, use the arrow keys to move the cursor to "P" and press the center button.



7 If the reader displays ">Range", dilute filtered extract by pipetting 400 µL of 70% MeOH to a new strip test vial. Then, using the same tip, add 100 µL of the filtered extract to the vial and mix well by vortexing



8 Repeat steps 4–6 with the diluted extract and multiply the displayed result by 5 to obtain the true level of contamination.

9 To run the next sample, use the arrow keys to move the cursor to "NT" and press the center button on the keypad.



Orders:
Tel: +1-877.228.4244
+1-417.725.6588
Email: orders@vicam.com

Technical Support:
Tel: +1.800.338.4381
+1.508.482.4935
Email: techservice@vicam.com

715006796 Rev A 1H

©2024 Waters Corporation. Waters, Afla-V, VICAM, and VERTU are trademarks of Waters Corporation.

WatersTM | VICAMTM

www.vicam.com