

Guided

Zirconia Implants:

in Complex Anatomical Sites



What to Expect

Abstract:

The clinical application of modern bio ceramics has evolved beyond simple prosthetic restorations. Today, Zirconia is successfully utilized as a primary dental implant material, enabling a comprehensive, metal-free restoration concept. However, the inherent material properties of zirconia, coupled with patient-specific anatomical challenges, demand a higher level of surgical precision. This case study examines the clinical journey of a patient with metal sensitivities and limited bone density, highlighting the transition from traditional protocols to a guided zirconia implant placement using the **ITX** Universal Guided Kit.

The Clinical Challenge:

A male patient presented with missing anterior teeth (#9# ,8# ,7, and #10). The site was previously diagnosed as "inadequate for implants" due to bone loss and sinus pneumatization.

Key Constraints:

1. **Bone Deficiency:** Previous consultations suggested that extensive bone grafting was mandatory
2. **Metal Sensitivity:** The patient expressed strong concerns regarding metal biocompatibility and requested a non-metallic alternative.
3. **Aesthetic Requirements:** Concern over potential "graying" of the gingiva—a common side effect of titanium in patients with a thin biotype.

The Biological Advantage of Zirconia

One of the key biological advantages of zirconia is its ability to maintain natural gingival aesthetics, even in patients with a thin biotype. *Unlike* titanium, which can cast a gray shadow through the gums, the white color of zirconia ensures a seamless transition between the implant and the crown. While titanium remains an option for aesthetic sites, it necessitates a 'safety zone' of at least soft tissue thickness to prevent the metallic color from compromising the final smile.¹

Clinical observations also show that soft tissue around zirconia is "happier." *Unlike* the hemidesmosome connection seen with titanium, zirconia allows for a true epithelial attachment, creating a biological seal that is more resistant to bacterial infiltration and recession.²

Like all metals, Titanium is subject to corrosion, and therefore, they release micro-particles through corrosion and abrasion, triggering a chronic inflammatory response known as "titanium intolerance." This intolerance is considered to be a non-specific macrophage reaction.³

Notably, a true Type IV "titanium allergy" is physiologically impossible because released titanium ions instantly react with oxygen to form stable titanium dioxide—a ceramic passivation layer that prevents the formation of immunologically reactive haptens.⁴

Although rare, reported titanium allergic reactions are frequently caused by manufacturing impurities such as nickel or alloying elements found in Grade V titanium, such as vanadium and aluminum, which can be released in ionic form. To mitigate these immunological risks, zirconium dioxide offers a superior alternative due to its bio-inert properties.⁵

Unlike metals, zirconia does not undergo chemical or biological interactions with host tissue, ensuring that no toxic or allergenic substances are released into the system. This stability eliminates the possibility of sensitization or immunological rejection, making zirconia the ideal material for a metal-free restorative concept and rendering preoperative intolerance testing for ceramics unnecessary.⁴

The Mechanical Advantage of Zirconia:

The bio-inert nature of zirconia is a direct result of its classification as a ceramic. While the base element, zircon, is a metal, a complete and irreversible oxidation process converts it into zirconium dioxide. This chemical transition creates a fundamental difference in reactivity: *unlike* titanium, which contains free and highly reactive electrons, the electrons in zirconium dioxide are secured within stable covalent bonds. This lack of free electrons renders the material chemically non-reactive, ensuring it does not engage in destructive interactions with surrounding biological tissues.⁶

This low reactivity provides several unique clinical benefits, including minimal surface tension, low solubility, and complete resistance to the corrosion typically seen in metallic implants. Furthermore, zirconia exhibits low thermal and electrical conductivity, which enhances its compatibility with sensitive peri-implant environments. However, these ceramic properties also present a mechanical trade-off; the material lacks the elasticity of metal, resulting in a higher inherent susceptibility to fracture compared to titanium systems.⁴

Advancements in material engineering have led to a dramatic reduction in ceramic implant fracture rates, dropping from 3.4% to just 0.2%.⁷

Both static and dynamic testing, as outlined in ISO 14801 standards, confirm that contemporary ceramic systems possess the mechanical strength necessary for reliable clinical applications. However, stability is not determined by the material alone; the **European Society for Ceramic Implantology** emphasizes that specific manufacturing techniques, implant geometry, and the design of the prosthetic connection also influence the mechanical integrity of two-piece implants.^{8,9}

Comparison between Titanium and Zirconium dental implants.²

Feature	Titanium	Zirconium
<i>Biocompatibility</i>	Lesser biocompatibility; it releases metal ions over time, leading to a mild inflammatory response.	Higher biocompatibility; doesn't corrode or release ions.
<i>Integration & History</i>	Long history of successful use providing excellent osseointegration.	Excellent soft tissue integration, yet short history in use.
<i>Hygiene</i>	More prone to bacterial adhesion.	Less prone to bacterial adhesion.
<i>Aesthetics</i>	Aesthetic concerns; titanium's metallic color can sometimes be visible through the gum tissue.	More aesthetically pleasing; the white color of zirconium blends better with the surrounding teeth.



The ITXPROS Advantage:

Why Guided?

While the material provides the biological foundation, **Guided Surgery** provides the execution. For ceramic implants, where primary stability and restorative-driven placement are critical, **ITXPROS** digital planning acts as the bridge between theory and clinical success.

Restorative-driven implantology is now a standard reality, where virtual planning allows for the exact determination of a fixture's orientation.^{10,11}

By utilizing high-accuracy **surgical guides**, clinicians can replicate these digital designs chairside, ensuring that every implant is placed at the optimized depth and angle for long-term success. The advantages of **guided surgery** include greater precision, reduced trauma to the patient, and reduced duration of the surgical procedure. **Guided surgery** is indicated in situations of critical anatomy, such as proximity to the inferior dental nerve or maxillary sinus, as it offers greater precision and a lower probability of complications.¹²

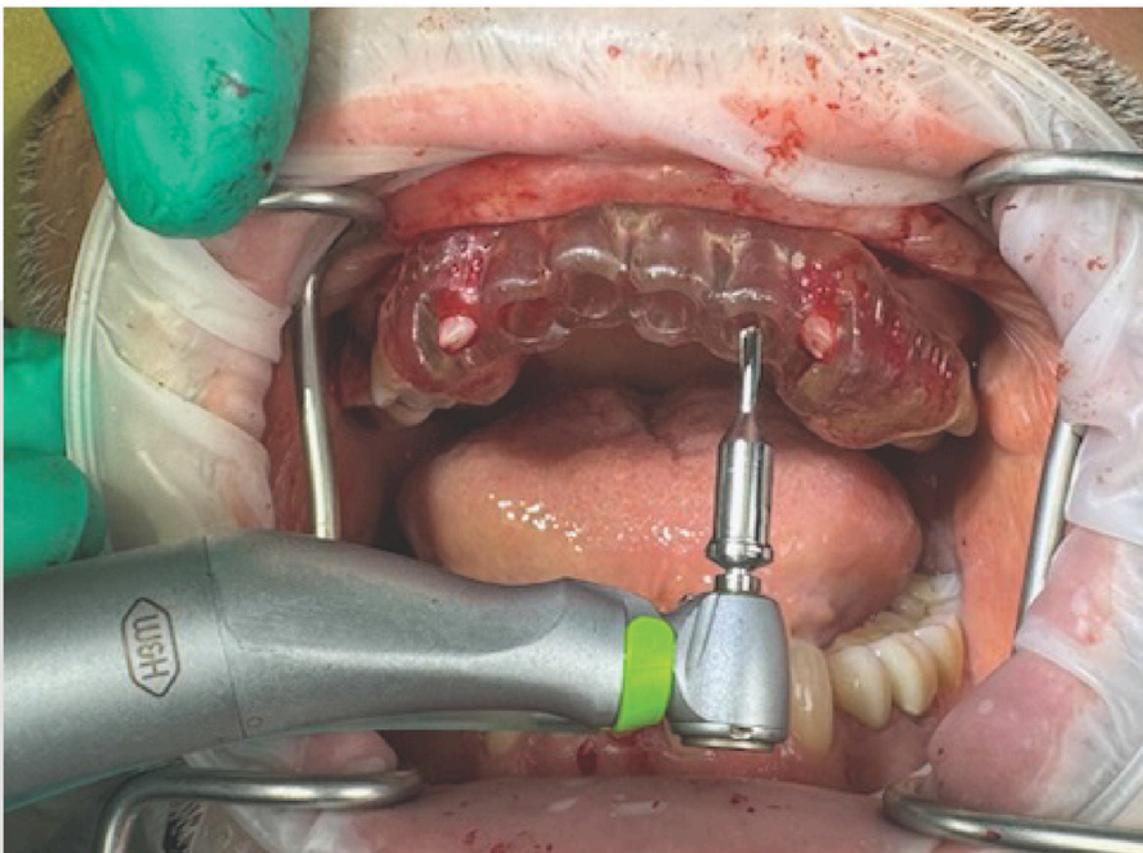


Fig.1.
ITXPROS Tooth-supported surgical guide in action.

Step-by-Step Surgical Execution:

To ensure predictability in a bone-compromised site, **Dr. Assi** utilized **Guided Surgery** protocols. A significant hurdle in ceramic implantology is that many zirconia systems lack proprietary guided kits.

1- Reverse Engineering:

The team started with the final prosthesis design, working backward to place the implant. This "restorative-driven" approach ensures that the implant is not just "in bone," but in the perfect position for the final prosthesis.

2- Guided Precision in Limited Bone:

With sinus pneumatization present, the margin for error was near zero.

The **ITXPROS** guide allowed for:

Predictability: Placement matched the virtual plan exactly.

Efficiency: Reduced surgical time by an estimated 30%, directly correlating to 4% reduction in morbidity per minute saved.

3- Clinical Results & Success Metrics:

Metric	Clinical Goal	Achieved Result
Insertion Torque	> 35 NM	45 NM
ISQ Value (Stability)	> 68	72
Soft Tissue Response	Pink, non-inflamed	Healthy, natural attachment
Aesthetics	No gray shadowing	Seamless white-to-pink transition

Fig.2. Immediate post-operative results after implant placement.



a. before suturing.



b. after suturing.

REFERENCES LIST:

- 1- Jung RE, Sailer I, Hämmerle CH, Attin T, Schmidlin P. In vitro color changes of soft tissues caused by restorative materials. *Int J Periodontics Restorative Dent*. Jun 2007;27(3):251-7.
- 2- Abouel Maaty FAN, Ragab MA, El-Ghazawy YM, et al. Peri-Implant Soft Tissue in Contact with Zirconium/Titanium Abutments from Histological and Biological Perspectives: A Concise Review. *Cells*. Jan 17 2025;14(2)doi:10.3390/cells14020129
- 3- Jacobi-Gresser E, Huesker K, Schütt S. Genetic and immunological markers predict titanium implant failure: a retrospective study. *Int J Oral Maxillofac Surg*. Apr 2013;42(4):537-43. doi:10.1016/j.ijom.2012.07.018
- 4- Tartsch J, Blatz MB. Ceramic Dental Implants: An Overview of Materials, Characteristics, and Application Concepts. *Compend Contin Educ Dent*. Sep 2022;43(8):482-488; quiz 489.
- 5- Harloff T, Hönle W, Holzwarth U, Bader R, Thomas P, Schuh A. Titanium allergy or not? "Impurity" of titanium implant materials. *Health*. 2010;2:306-310.
- 6- Kanchana S, Hussain S. Zirconia a bio-inert implant material. *IOSR J Dent Med Sci*. 2013;12(6):66-67.
- 7- Roehling S, Schlegel KA, Woelfler H, Gahlert M. Performance and outcome of zirconia dental implants in clinical studies: A meta-analysis. *Clin Oral Implants Res*. Oct 2018;29 Suppl 16:135-153. doi:10.1111/clr.13352.
- 8- Joda T, Voumard B, Zysset PK, Brägger U, Ferrari M. Ultimate force and stiffness of 2-piece zirconium dioxide implants with screw-retained monolithic lithium-disilicate reconstructions. *J Prosthodont Res*. Apr 2018;62(2):258-263. doi:10.1016/j.jpor.2017.11.002.
- 9- pies BC, Fross A, Adolfsson E, Bagegni A, Doerken S, Kohal RJ. Stability and aging resistance of a zirconia oral implant using a carbon fiber-reinforced screw for implant-abutment connection. *Dent Mater*. Oct 2018;34(10):1585-1595. doi:10.1016/j.dental.2018.08.290.
- 10- Mora MA, Chenin DL, Arce RM. Software tools and surgical guides in dental-implant-guided surgery. *Dent Clin North Am*. Jul 2014;58(3):597-626. doi:10.1016/j.cden.2014.04.001.
- 11- Jung RE, Schneider D, Ganeles J, et al. Computer technology applications in surgical implant dentistry: a systematic review. *Int J Oral Maxillofac Implants*. 2009;24 Suppl:92-109.
- 12- Araujo-Corchado E, Pardal-Peláez B. Computer-guided surgery for dental implant placement: a systematic review. *Prosthesis*. 2022;4(4):540-553.

