

HCR™ Pro RNA-ISH Setup Guide for the BOND-III

This Setup Guide demonstrates the use of an HCR™ Pro RNA-ISH kit on the BOND-III platform from Leica Biosystems. Reagent preparation steps, including registering individual BOND Containers for their respective reagents, will be described in further detail. Each BOND-III run takes approximately 13-14.5 hours followed by a short post-processing of stained slides. This time range depends on the number of slides processed in a single run. Processing 5 slides takes around 13 hours, and processing 30 slides takes around 14.5 hours due to the time the BOND-III platform takes to disperse the reagents onto each slide. The HCR™ Pro RNA-ISH kit can be used to probe and visualize RNA transcripts in FFPE tissue sections. Please read through the Setup Guide for additional information so that you can easily incorporate the HCR™ Pro RNA-ISH kit into your current workflow.

Table of Contents

HCR™ Pro RNA-ISH Kit Information	2
<i>HCR™ Pro RNA-ISH Kit</i>	2
<i>HCR™ HiFi Probe</i>	2
<i>HCR™ Pro Detect.....</i>	2
<i>Required Materials for BOND-III</i>	3
<i>User-Supplied Materials</i>	4
Overall Workflow of the HCR™ Pro RNA-ISH Protocol	5
Set Up BOND-III Protocols	6
<i>Register BOND Containers.....</i>	6
<i>Registering a New Reagent</i>	8
<i>Create Staining Protocols for HCR™ Pro RNA-ISH</i>	10
<i>HCR™ HiFi Probe 1A Registration</i>	11
<i>Set Up Slides and Print Labels</i>	12
<i>Post-Processing for AP-Based Detection</i>	13
<i>Post-Processing for HRP-Based Detection.....</i>	13
Reagent Preparation	14
<i>Reagent Transfer and Storage</i>	14
Overall Workflow of the HCR™ Pro RNA-ISH + IHC Protocol.....	16
HCR™ Pro RNA-ISH + IHC Co-Detection Protocol.....	17
<i>Set Up Slides with Two Sequential Staining Protocols</i>	17

HCR™ Pro RNA-ISH Kit Information

Upon receiving an HCR™ Pro RNA-ISH Kit, please check all reagents and their storage conditions.

HCR™ Pro RNA-ISH Kit

The HCR™ Pro RNA-ISH kit consists of an HCR™ HiFi Probe and HCR™ Pro Detect reagents. Each HCR™ HiFi Probe includes 2 components: (1) HCR™ HiFi Probe 1A and (2) HCR™ HiFi Probe 1B. The probes are provided ready-to-use and can be transferred directly to open containers for use or storage.

HCR™ HiFi Probe

HCR™ Reagents	Amount for 20 Slides	Amount for 90 Slides	Storage Temperature
HCR™ HiFi Tissue Stabilizer	7 mL	29 mL	2 to 8 °C
HCR™ HiFi Probe 1A ¹	7 mL	29 mL	2 to 8 °C
HCR™ HiFi Probe 1B ¹	7 mL	29 mL	2 to 8 °C

¹HCR™ HiFi Probes are platform-specific. For example, probes designed for the BOND RX autostainer are not compatible with the BOND-III, and vice versa.

HCR™ Pro Detect

Please note that all HCR™ Pro Detect reagents are provided in amber bottles, as these reagents are sensitive to light.

HCR™ Reagents	Amount for 20 Slides	Amount for 90 Slides	Storage Temperature
Pretreat	5 mL	21 mL	2 to 8 °C
HCR™ Pro Detect A	5 mL	21 mL	2 to 8 °C
HCR™ Pro Detect B	7 mL	29 mL	2 to 8 °C
HCR™ Pro Detect C	5 mL	21 mL	2 to 8 °C
HCR™ Pro Detect D	7 mL	29 mL	2 to 8 °C
HCR™ Pro Detect E	7 mL	29 mL	2 to 8 °C
HCR™ Pro Detect F AP/HRP ¹	7 mL	29 mL	2 to 8 °C
Post-Process A	5 mL	21 mL	2 to 8 °C
Post-Process B ²	7 mL	29 mL	2 to 8 °C

¹HCR™ Pro Detect F AP is included in the HCR™ Pro RNA-ISH AP kit, and HCR™ Pro Detect F HRP is included in the HCR™ Pro RNA-ISH HRP kit.

²Post-Process B is only needed if you are performing an HCR™ Pro RNA-ISH + IHC co-detection assay.

Required Materials for BOND-III

The HCR™ Pro RNA-ISH protocol requires specific materials available only from Leica Biosystems (LBS). It is essential to check the availability of these materials prior to setting up an HCR™ Pro RNA-ISH experiment. For more information, please inquire with your Leica Biosystems representative.


Materials from Leica Biosystems		
	Catalog #	Storage Temperature
BOND 6 mL Titration Kit	OPT9049	RT
BOND 7 mL Open Container	OP79193	RT
BOND Universal Covertiles 160 Pack	S21.4611	RT
BOND Epitope Retrieval Solution 2	AR9640	2 to 8 °C
BOND Dewax Solution	AR9222	2 to 26 °C
BOND Wash Solution 10X Concentrate	AR9590	2 to 8 °C
BOND Polymer Refine Red Detection ¹	DS9390	2 to 8 °C
BOND Polymer Refine Detection ¹	DS9800	2 to 8 °C
BOND Mixing Stations	S21.1971	RT

¹The HCR™ Pro RNA-ISH protocol uses Fast Red/DAB chromogens and hematoxylin from the BOND Polymer Refine Red Detection kit or the BOND Polymer Refine Detection kit for chromogenic deposition and counterstain. The HCR™ Pro RNA-ISH AP kit requires the use of the BOND Polymer Refine Red Detection kit, and the HCR™ Pro RNA-ISH HRP kit requires the use of the BOND Polymer Refine Detection kit.

User-Supplied Materials

Materials from Other Vendors		
	Supplier	Comment
FFPE Sample Slides	Any	SuperFrost or SuperFrost® Plus slides are recommended for best results
Propar (xylene substitute)	Fisher Scientific	Xylene may be substituted
Drying Oven	Any	Capable of maintaining temperature at ~60 °C
BioCare EcoMount, Leica CV Ultra Mounting Media, or Vectorlabs VectaMount	BioCare, Leica Biosystems, and Vectorlabs	Mounting medium compatible with all LBS chromogens
Cytoseal	Any	Suitable mounting medium for HRP-driven chromogens
Cover Glass	Any	Dimension depends on the size of the tissue
100% Ethanol	Any	None

Overall Workflow of the HCR™ Pro RNA-ISH Protocol

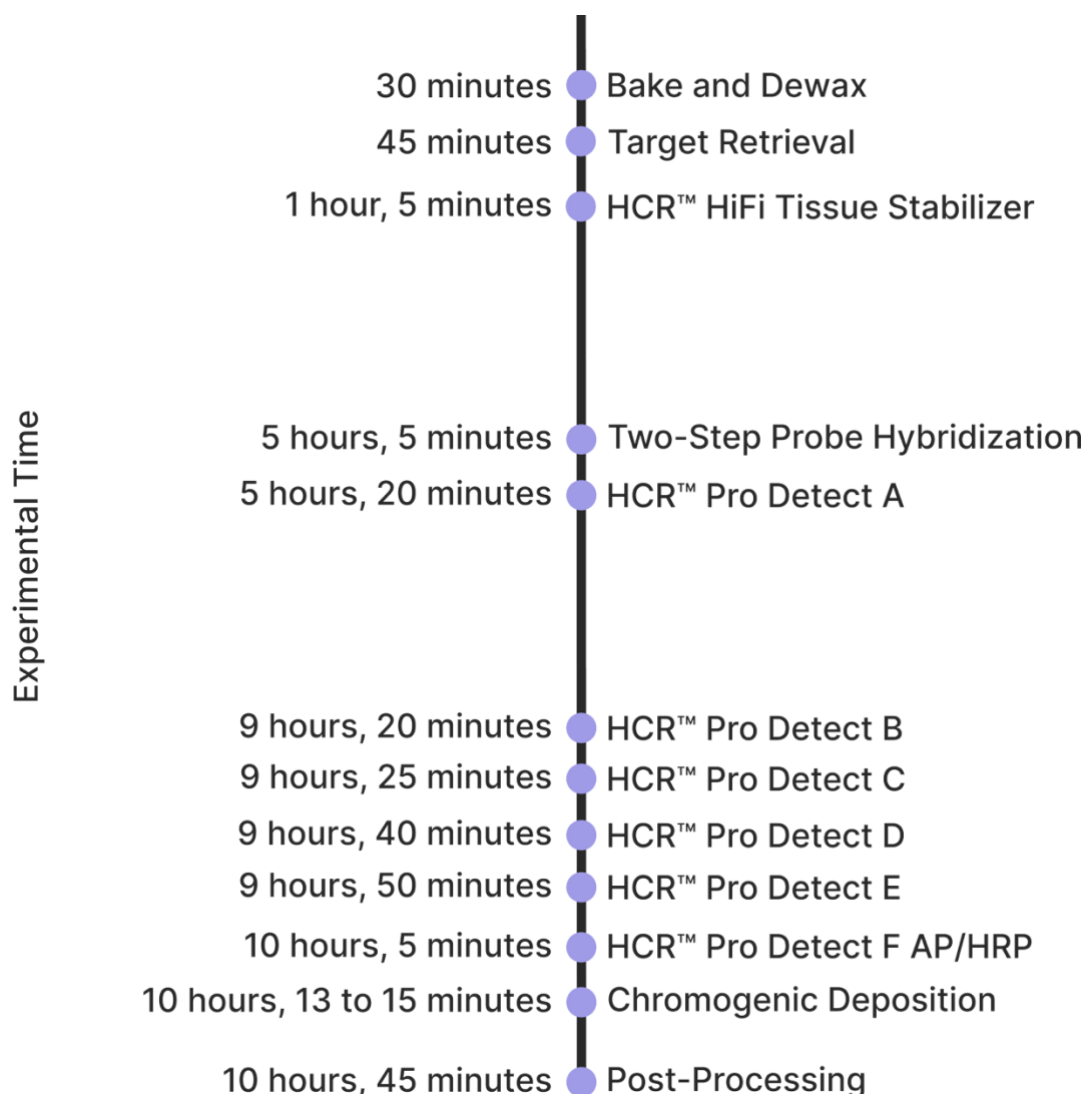

As mentioned earlier, each BOND-III run takes approximately 13 to 14.5 hours. The timeline above only accounts for 10 hours and 45 minutes of this run, as the remaining time comes from the additional BOND-III washing steps.

Set Up BOND-III Protocols

The HCR™ Pro RNA-ISH assay utilizes an IHC protocol to employ a two-step probe hybridization approach. HCR™ HiFi Probe A and Probe B are registered as the reagent types “primary antibody” and “ancillary,” respectively. As a result, HCR™ HiFi Probe A will be denoted as *Marker and HCR™ HiFi Probe B will retain its name in the staining protocol. *Please note that a separate protocol is needed for every target probe (e.g., two separate staining protocols are needed for running DapB and PPIB probes).*

The five main steps in setting up a BOND-III protocol for an HCR™ Pro RNA-ISH run are:

- i. Register BOND Containers associated with their respective reagents (if needed)
- ii. Create a staining protocol for your custom probe(s) using an existing HCR™ Pro RNA-ISH protocol
- iii. Register your custom HCR™ HiFi Probe A(s) as primary antibodies
- iv. Set up slides and print labels

Register BOND Containers

In order to create an HCR™ Pro RNA-ISH protocol on the BOND-III, reagent names associated with the BOND Containers must be registered in the BOND-III software. The table below lists all the BOND Containers that need to be registered for the HCR™ Pro RNA-ISH assay.

BOND Containers			
Name	Type of Container ¹	Type of Reagent	Reagent Registration required?
*Enzyme 2 ²	7 mL or 30 mL BOND Container	N/A	No
HCR™ HiFi Tissue Stabilizer	7 mL or 30 mL BOND Container	Ancillary	Yes
HCR™ HiFi Probe 1A	6 mL, 7 mL, or 30 mL Container	Primary antibody ³	Yes
HCR™ HiFi Probe 1B	6 mL, 7 mL, 30 mL Container	Ancillary	Yes
HCR™ Pro Detect A	7 mL or 30 mL BOND Container	Ancillary	Yes
HCR™ Pro Detect B	7 mL or 30 mL BOND Container	Ancillary	Yes
HCR™ Pro Detect C	7 mL or 30 mL BOND Container	Ancillary	Yes
HCR™ Pro Detect D	7 mL or 30 mL BOND Container	Ancillary	Yes
HCR™ Pro Detect E	7 mL or 30 mL BOND Container	Ancillary	Yes
HCR™ Pro Detect F AP/HRP	7 mL or 30 mL BOND Container	Ancillary	Yes

Post-Process A	7 mL or 30 mL BOND Container	Ancillary	Yes
*Enzyme 1 ⁴	7 mL or 30 mL BOND Container	Ancillary	Yes

¹We recommend using 7 mL and 30 mL BOND Containers for 20-slide and 90-slide kits, respectively.


²While the *Enzyme 2 reagent does not require registration since it is a pre-existing reagent found in the software, the BOND Container itself does need to be registered. Please note that the BOND Container for *Enzyme 2 will hold the Pretreat reagent (reference page 14).

³Even though the reagent type, Primary antibody, is used, the Container will need to be filled with HCR™ HiFi Probe 1A Solution.

⁴While the *Enzyme 1 reagent does not require registration since it is a pre-existing reagent found in the software, the BOND Container itself does need to be registered. Please note that the BOND Container for *Enzyme 1 will hold the Post-Process B reagent (reference page 14). This reagent is only required for running an HCR™ Pro RNA-ISH + IHC co-detection assay.

Registering a New Reagent

- From the top navigation bar, click on **Reagent setup** at the top of the screen and select **Add**.

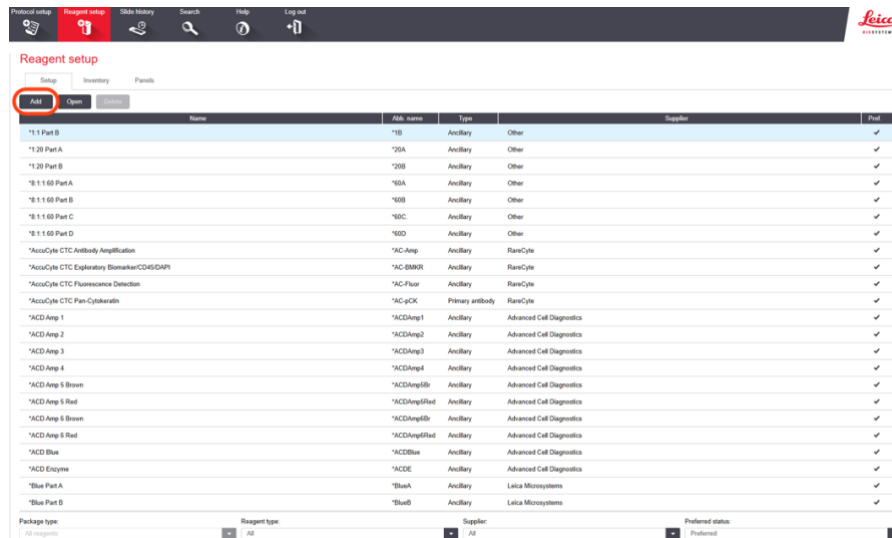

Reagent setup

Setup Inventory Panels

Add Open Cancel

Name	Abb. name	Type	Supplier	Prod
*1.1 Part B	*1B	Ancillary	Other	✓
*1.20 Part A	*20A	Ancillary	Other	✓
*1.20 Part B	*20B	Ancillary	Other	✓
*1.1.60 Part A	*60A	Ancillary	Other	✓
*1.1.60 Part B	*60B	Ancillary	Other	✓
*1.1.60 Part C	*60C	Ancillary	Other	✓
*1.1.60 Part D	*60D	Ancillary	Other	✓
*AccuCyte CTC Antibody Amplification	*AC-Amp	Ancillary	RareCyte	✓
*AccuCyte CTC Exploratory Biomarker CD45/DAPI	*AC-BMNR	Ancillary	RareCyte	✓
*AccuCyte CTC Fluorescence Detection	*AC-Fluo	Ancillary	RareCyte	✓
*AccuCyte CTC Pan-Cytokeratin	*AC-pCK	Primary antibody	RareCyte	✓
*ACD-Amp 1	*ACDAmp1	Ancillary	Advanced Cell Diagnostics	✓
*ACD-Amp 2	*ACDAmp2	Ancillary	Advanced Cell Diagnostics	✓
*ACD-Amp 3	*ACDAmp3	Ancillary	Advanced Cell Diagnostics	✓
*ACD-Amp 4	*ACDAmp4	Ancillary	Advanced Cell Diagnostics	✓
*ACD-Amp 5 Brown	*ACDAmp5Br	Ancillary	Advanced Cell Diagnostics	✓
*ACD-Amp 5 Red	*ACDAmp5Red	Ancillary	Advanced Cell Diagnostics	✓
*ACD-Amp 6 Brown	*ACDAmp6Br	Ancillary	Advanced Cell Diagnostics	✓
*ACD-Amp 6 Red	*ACDAmp6Red	Ancillary	Advanced Cell Diagnostics	✓
*ACD-Blue	*ACDBlue	Ancillary	Advanced Cell Diagnostics	✓
*ACD-Enzyme	*ACDE	Ancillary	Advanced Cell Diagnostics	✓
*Blue Part A	*BlueA	Ancillary	Leica Microsystems	✓
*Blue Part B	*BlueB	Ancillary	Leica Microsystems	✓

Package type: All reagents Reagent type: AS Supplier: AS Preferred status: Preferred

- The following screenshot is an example of how to add an Ancillary reagent. Check the **Preferred** box and click **Save**.

Note: Since the default staining cannot be left blank during registration, the HCR™ HiFi Probe 1A reagent can only be added after the ancillary reagents and staining protocols have been added to the BOND-III software.

X

Add reagent

Name:

Abbreviated name:

Type: ▼

Supplier:

Available bulks:

>>

<<

Compatible bulks:

*BWash

*DI

☒ Preferred ☐ Hazardous

Save Cancel

3. To register a BOND Container (e.g., BOND Open Container) with an associated reagent, scan the barcode on the container, which will prompt the following screen. Select the **reagent name** that was created previously. Add an **expiration date** far into the future as the BOND Container can be reused. Click **OK**.

×

Add open container

Bond Open Container, 7 mL
Catalog N°: OP79172 UPI: 19035337
Supplier: Leica Microsystems

Reagent name

HCR Pro Detect A (Molecular Instruments) ▼

Lot N°:

Expiration date:

📅

Initial vol. (mL)

7.00

OK

Cancel

4. Repeat Steps 1-3 for all the required reagents.

Create Staining Protocols for HCR[™] Pro RNA-ISH

1. From the top navigation bar, click on **Protocol setup** on the top of the screen and select **Staining** for the protocol group. Select a previous HCR[™] Pro RNA-ISH protocol, and click on the **Copy** button near the top-right corner.
2. Change the name to **HCR[™] RNA-ISH AP (or HRP)- custom probe** and enter your preferred **Abbreviated name**. It's important to note that each probe requires a separate staining protocol.
3. Replace the two previous Probe 1B steps with that of your current custom Probe 1B.
4. For AP and HRP-based detection, please select "**BOND Polymer Refine Red Detection**" and "**BOND Polymer Refine Detection,**" respectively, as the **Preferred detection system** for the protocol. Click **Save**. Ensure that the **Preferred** box has been checked before saving.

HCR™ HiFi Probe 1A Registration

Now that all of the necessary reagents and their respective BOND Containers have been registered and assigned to our protocols, we can register the HCR™ HiFi Probe 1A BOND Container.

1. Similarly to the other reagent registration processes, click on **Reagent setup** from the top navigation bar and select **Add**.
2. Enter the probe **Name**, **Abbreviated name**, **Type** (Primary antibody), and **Supplier** (Molecular Instruments). Then, use the drop-down menus to select the previously created **Default staining**, **HIER**, and **enzyme** protocols. Make sure the **Preferred** box is selected. Two examples of registering HCR™ HiFi Probe A (e.g., DapB and PPIB) are shown below.

*Note that the probe specified in the default staining protocol must match the target listed under **Name**; mismatches can cause programming errors and result in dispensing the wrong probe reagent.*

DapB:

Add reagent

Name: HCR HiFi Probe A (DapB)

Abbreviated name: HCRdapB

Type: Primary antibody

Supplier: Molecular Instruments

Single/double stain: Single/Sequential DS

Single First Second

Default staining protocol: HCR Pro RNA-ISH AP - DapB

Default HIER protocol: HCR Target retrieval 15 min at 95C

Default enzyme protocol: Pretreat

Compatible bulks:
*BWash

☒ Preferred ☐ Hazardous

Save Cancel

PPIB:

Add reagent

Name: HCR HiFi Probe A (PPIB)

Abbreviated name: HCRAPPIB

Type: Primary antibody

Supplier: Molecular Instruments

Single/double stain: Single/Sequential DS

Single First Second

Default staining protocol: HCR Pro RNA-ISH AP - PPIB

Default HIER protocol: HCR Target retrieval 15 min at 95C

Default enzyme protocol: Pretreat

Compatible bulks:
*BWash

☒ Preferred ☐ Hazardous

Save Cancel

Set Up Slides and Print Labels

- From the top navigation bar, click on **Slide setup** on the top of the screen and select **Add study**. Enter **Study ID**, **Study name**, and **Study comments**. Select ***Bake and Dewax** for the **Preparation protocol**. Click **OK**.

- Click on **Add slide**. In this example, **HCR™ HiFi Probe A (DapB)** is selected as the **Marker**. If you registered the probe as described in the previous section, the associated protocols will self-populate. You can select a different probe as needed based on your RNA target of interest.

3. For additional slides, keep this window open, change the parameters as needed, and then click **Add slide**. Continue until all slides have been added, then click **Close**.
4. After all the slides have been added, click on **Print labels**, select **All slide labels not yet printed for the current study**, and click **Print**.
5. Peel off the labels and attach them individually to the top portion (white region) of the slides.

Post-Processing for AP-Based Detection

After slides are unloaded from the BOND-III, we recommend rinsing the slides with Deionized water. Bake the slides for 15 minutes (or until dry) at 60 °C. We recommend using either the EcoMount (Biocare), VectaMount (Vectorlabs), or Leica CV Ultra mounting media for cover-slipping.

Post-Processing for HRP-Based Detection

After slides are unloaded from the BOND-III, we recommend rinsing the slides with Milli-Q water. Dehydrate by immersing the slides in 95% ethanol for 3 minutes twice followed by 100% ethanol for 3 minutes. Then, immerse the slides in a xylene (or xylene substitute) solution for 5 minutes and mount one slide at a time with Cytoseal (or any other xylene-based mounting medium). Allow slides to air dry for 5 minutes before imaging.

Reagent Preparation

Reagent Transfer and Storage

Instructions for reagent transfer can be found in the table below. Please transfer all HCR™ Pro RNA-ISH reagents to their name-associated containers. Please store all BOND Containers in a 4 °C fridge after use.


BOND Container	Instructions	Storage Conditions
*Enzyme 2	Transfer entirety of Pretreat to the BOND Container	Store at 4 °C after use
HCR™ HiFi Tissue Stabilizer	Transfer entirety of HCR™ HiFi Tissue Stabilizer to the 7 mL or 30 mL BOND Container	Store at 4 °C after use
HCR™ HiFi Probe 1A	Transfer the entirety of HCR™ HiFi Probe 1A Solution to the 6 mL, 7 mL, or 30 mL BOND Container	Store at 4 °C after use
HCR™ HiFi Probe 1B	Transfer the entirety of HCR™ HiFi Probe 1B Solution to the 6 mL, 7 mL, or 30 mL BOND Container	Store at 4 °C after use
HCR™ Pro Detect A	Transfer entirety of HCR™ Pro Detect A to the 7 mL or 30 mL BOND Container	Store at 4 °C after use
HCR™ Pro Detect B	Transfer entirety of HCR™ Pro Detect B to the 7 mL or 30 mL BOND Container	Store at 4 °C after use
HCR™ Pro Detect C	Transfer entirety of HCR™ Pro Detect C to the 7 mL or 30 mL BOND Container	Store at 4 °C after use
HCR™ Pro Detect D	Transfer entirety of HCR™ Pro Detect D to the 7 mL or 30 mL BOND Container	Store at 4 °C after use
HCR™ Pro Detect E	Transfer entirety of HCR™ Pro Detect E to the 7 mL or 30 mL BOND Container	Store at 4 °C after use
HCR™ Pro Detect F AP	Transfer entirety of HCR™ Pro Detect F AP to the 7 mL or 30 mL BOND Container	Store at 4 °C after use
HCR™ Pro Detect F HRP	Transfer entirety of HCR™ Pro Detect F HRP to the 7 mL or 30 mL BOND Container	Store at 4 °C after use
Post-Process A	Transfer entirety of Post-Process A to the 7 mL or 30 mL BOND Container	Store at 4 °C after use
*Enzyme 1 ¹	Transfer entirety of Post-Process B to the 7 mL or 30 mL BOND Container	Store at 4 °C after use

¹The registration and filling of this reagent is only required for running an HCR™ Pro RNA-ISH + IHC co-detection assay.

Other important notes:

1. Please avoid excessive bubbles when transferring HCR[™] HiFi Probe and HCR[™] Pro Detect Solutions to the 7 mL or 30 mL BOND Open Containers.
2. If the reagent-filled BOND Containers have not been used for more than a week, it is highly recommended to gently invert the BOND Containers several times with the lid closed to ensure solution uniformity before next use.

Overall Workflow of the HCR™ Pro RNA-ISH + IHC Protocol

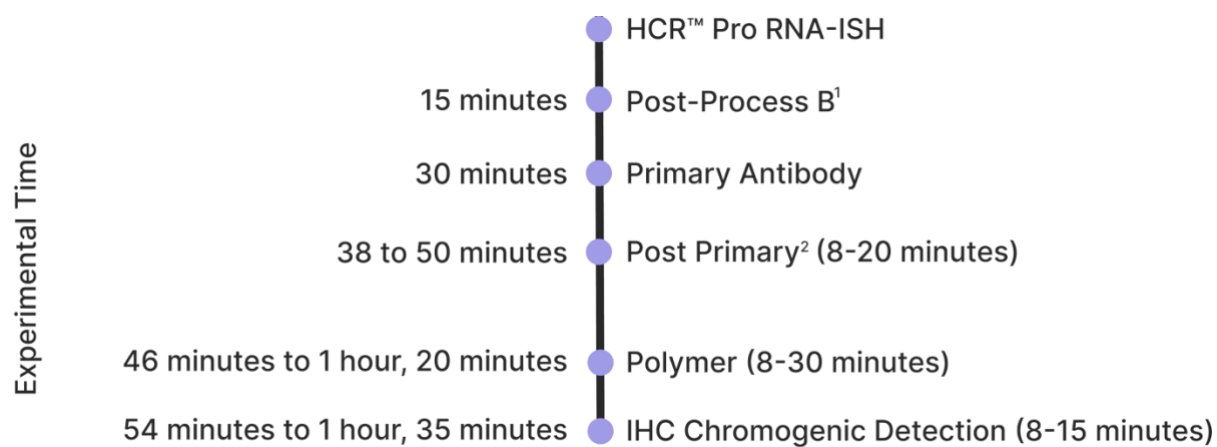

¹This step is NOT needed if HCR™ Pro RNA-ISH HRP detection is followed by IHC AP detection.

²This step is NOT needed if the species of the primary antibody used is rabbit.

HCR™ Pro RNA-ISH + IHC Co-Detection Protocol

Set Up Slides with Two Sequential Staining Protocols

1. From the top navigation bar, click on **Slide setup** on the top of the screen and select **Add study**. Enter **Study ID**, **Study name**, and **Study comments**. Select ***Bake and Dewax** for the **Preparation protocol**. Click **OK**.
2. Click on **Add slide**, change the **Staining mode** to **Sequential DS**. Under the **First** tab, select IHC and proceed with the selections for running an HCR™ Pro RNA-ISH protocol with the new hematoxylin-free HCR™ Pro RNA-ISH protocol you created previously.

Slide properties

PPIB + CD3 IHC

Tissue type: ☒ Test tissue ☐ Negative tissue ☐ Positive tissue

Dispense volume: ☐ 100 µL ☒ 150 µL

Staining mode: Sequential DS

First Second

Process: ☒ IHC ☐ ISH

Marker: HCR HiFi Probe A (PPIB) (Molecular Instruments)

Protocols

Staining: HCR Pro RNA-ISH AP – PPIB No hematoxylin

Preparation: *Bake and Dewax

HIER: HCR Target retrieval 15 min at 95C

Enzyme: Pretreat

OK Copy slide Close

3. Select the **Second** tab and use the previously modified IHC protocol as the **Staining** protocol. Then, select **Post-Process B** as the **Enzyme** protocol. Click **Add slide**.

Slide properties

PPIB + CD3 IHC

Tissue type: ☒ Test tissue ☐ Negative tissue ☐ Positive tissue

Dispense volume: ☐ 100 µL ☒ 150 µL

Staining mode: Sequential DS

First Second

Process: ☒ IHC ☐ ISH

Marker: *CD3 (LN10)

Protocols

Staining: IHC Protocol F (second)

HIER: *

Enzyme: Post-Process B

OK Copy slide Close

Important Notes:

1. ***Enzyme 2** is used for Pretreat in the first sequence, and ***Enzyme 1** is used for Post-Process B in the second sequence.
2. If **HRP-based RNA-ISH** detection is followed by **AP-based IHC**, the Enzyme protocol in the second sequence is **not** required and should be left blank.
3. If a red chromogen is used for either ISH or IHC detection, slides cannot be dehydrated in alcohol. Instead, bake the slides for ~30 minutes or allow them to air-dry overnight prior to mounting.