



POMTM Procedural Oxygen Mask[®]

Safety. Simplicity. Innovation.
All in the same breath.

Now
available in
medium

You and your patients can now breathe easier. We're bringing an innovative solution for oxygen delivery during procedures requiring sedation* into our comprehensive portfolio.

Previously available via distributor, POM was a product you ordered.
Now, it comes with a partnership you can count on.


Available in three sizes:

- 1** Large
- 2** Medium
- 3** Small (pediatric)



POM accepts a wide range of scopes, probes, and tubes with ease, while also allowing for EtCO₂ monitoring.


Its unique design and versatility allow hassle-free insertion through the patient's mouth or nose to maintain maximal oxygen delivery (FiO₂ 77-95%) and help monitor a patient's respiratory rate.**,¹

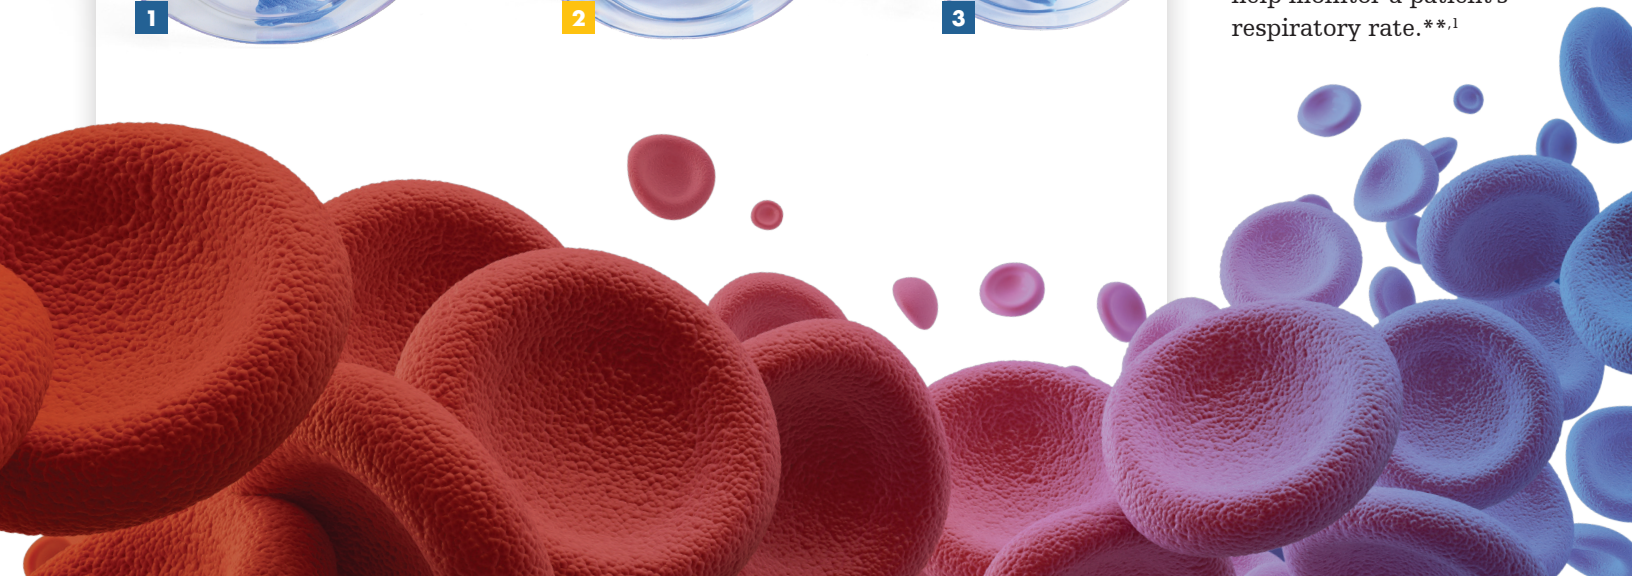

Product Description

Part Number

| | | | |
|----------------|--|----------------|--------------|
| 1 | Large Mask | | |
| | Mask, Medium/High Oxygen Concentration Adapter | | 1001 |
| | Mask, Medium/High Oxygen Concentration Adapter, 10ft Sampling Line | Male to Male | 1001-MM |
| | | Male to Female | 1001-MF |
| | | Microsteam | 1001-MSA |
| | Mask, Medium Oxygen Concentration Adapter | | 1003 |
| | Mask, Medium Oxygen Concentration Adapter, 10ft Sampling Line | Male to Male | 1003-MM |
| Male to Female | | 1003-MF | |
| Microsteam | | 1003-MSA | |
| 2 | Medium Mask | | |
| | Mask, Medium/High Oxygen Concentration Adapter | | 1001-MED |
| | Mask, Medium/High Oxygen Concentration Adapter, 10ft Sampling Line | Male to Male | 1001-MM-MED |
| | | Male to Female | 1001-MF-MED |
| | | Microsteam | 1001-MSA-MED |
| | Mask, Medium Oxygen Concentration Adapter | | 1003-MED |
| | Mask, Medium Oxygen Concentration Adapter, 10ft Sampling Line | Male to Male | 1003-MM-MED |
| Male to Female | | 1003-MF-MED | |
| Microsteam | | 1003-MSA-MED | |
| 3 | Small Mask (Pediatric) | | |
| | Mask, Medium/High Oxygen Concentration Adapter | | 1001-PED |
| | Mask, Medium/High Oxygen Concentration Adapter, 10ft Sampling Line | Male to Male | 1001-MM-PED |
| | | Male to Female | 1001-MF-PED |
| | | Microsteam | 1001-MSA-PED |
| | Mask, Medium Oxygen Concentration Adapter | | 1003-PED |
| | Mask, Medium Oxygen Concentration Adapter, 10ft Sampling Line | Male to Male | 1003-MM-PED |
| Male to Female | | 1003-MF-PED | |
| Microsteam | | 1003-MSA-PED | |

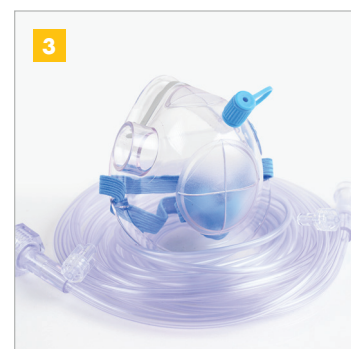

1 Sharma S, Danckers M, Sanghavi D, et al. High Flow Nasal Cannula. [Updated 2022 Sep 21]. In: StatPearls [Internet]. Treasure Island (FL): StatPearls Publishing; 2022 Jan-. Available from: <https://www.ncbi.nlm.nih.gov/books/NBK526071/>

*For non-intubated, spontaneously breathing patients

**For large size mask when compared to nasal cannulae or cutout standard oxygen masks.

Surgical Technologies

This document is intended solely for the use of healthcare professionals. A surgeon must always rely on his or her own professional clinical judgment when deciding whether to use a particular product when treating a particular patient. We do not dispense medical advice and recommend that surgeons be trained in the use of any particular product before using it in surgery.

The information presented is intended to demonstrate Stryker's products. A surgeon must always refer to the package insert, product label and/or instructions for use, including the instructions for cleaning and sterilization (if applicable), before using any of Stryker's products. Products may not be available in all markets because product availability is subject to the regulatory and/or medical practices in individual markets. Please contact your representative if you have questions about the availability of Stryker's products in your area.

Stryker or its affiliated entities own, use, or have applied for the following trademarks or service marks: POM Procedural Oxygen Mask, Procedural Oxygen Mask and Stryker. All other trademarks are trademarks of their respective owners or holders.

Stryker Instruments
1941 Stryker Way
Portage, MI 49002

[stryker.com](https://www.stryker.com)

ST-POM-BROC-1122776_REV-0
Copyright © 2024 Stryker

[safeOR.com](https://www.safeOR.com)