


NitriDerm®

Nitrile Exam Gloves Sterile Pairs Extended Cuff Series 114

Nitrile synthetic contains no natural rubber latex proteins. Soft, highly elastic formulation provides the maximum in comfort. Pair packaged, inner wrapper in ozone resistant multi-vac packaging.

Characteristics: Sterile, Powder-Free, Blue

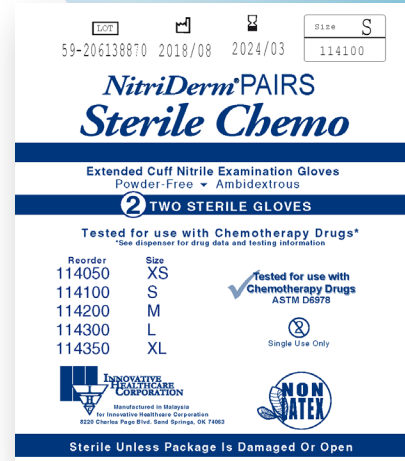

SIZE	ITEM NO.
XS	114050
S	114100
M	114200
L	114300
XL	114350

 **Tested for use with Chemotherapy Drugs**

All Sizes:
50 Pairs/Box, 4 Boxes/Case

Features:

- Textured Finger = an Improved Wet/Dry Grip
- Low Modulus = a Softer, More Comfortable Fit
- Non-Latex = No Risk of Latex Allergens
- Extended Cuff = Better Coverage

Manufactured in compliance with multiple international standards, including ASTM D6319, ASTM D5151, and ASTM F1671

Tested for use with Chemotherapy Drugs as per ASTM D6978 Standard Practice for Assessment of Medical Gloves to Permeation by Chemotherapy Drugs Minimum Breakthrough Detection Time in Minutes:			
Carmustine (BCNU) (3.3 mg/ml)	43.8	Fluorouracil (50.0 mg/ml)	>240
Cisplatin (1.0 mg/ml)	>240	Methotrexate (25.0 mg/ml)	>240
Cyclophosphamide (Cytoxan) (20.0 mg/ml)	>240	Mitomycin C (0.5 mg/ml)	>240
Dacarbazine (10.0 mg/ml)	>240	Paclitaxel (Taxol) (6.0 mg/ml)	>240
Doxorubicin Hydrochloride (2.0 mg/ml)	>240	Thio-Tepa (10.0 mg/ml)	97.8
Etoposide (Toposar) (20.0 mg/ml)	>240	Vincristine Sulfate (1.0 mg/ml)	>240

CAUTION: Please note Carmustine and Thiotepa have extremely low permeation times of 43.8 minutes and 97.8 minutes.

Caution: In compliance with ASTM D6978, the testing conditions used are intended to approximate the worst-case conditions for clinical use. Testing was conducted on single layer glove material. It is the users' responsibility to determine the applicability of these gloves for their intended use with chemotherapy drugs.

Tensile Strength & Elongation	Before Aging	After Accelerated Aging
Tensile Strength (Mpa)	32	33
ASTM Requirement Min. (Mpa)	14	14
Elongation (%)	691	667
ASTM Requirement Min. (%)	500	400

Average Length	11.5 in ♦ 290 mm
Average Palm Thickness	4.7 mil ♦ 0.12 mm
Average Finger Thickness	6.3 mil ♦ 0.16 mm



Innovative Healthcare Corporation is certified to ISO 13485:2016 QMS for medical devices.



Product Solutions You Trust

View this product on our website:

