


RD360™ DEVICE TECHNOLOGY GUIDE

READ THIS PRODUCT INSERT THOROUGHLY BEFORE USE

FIG. 1

RD360™ - THE RUNNING DEVICE®

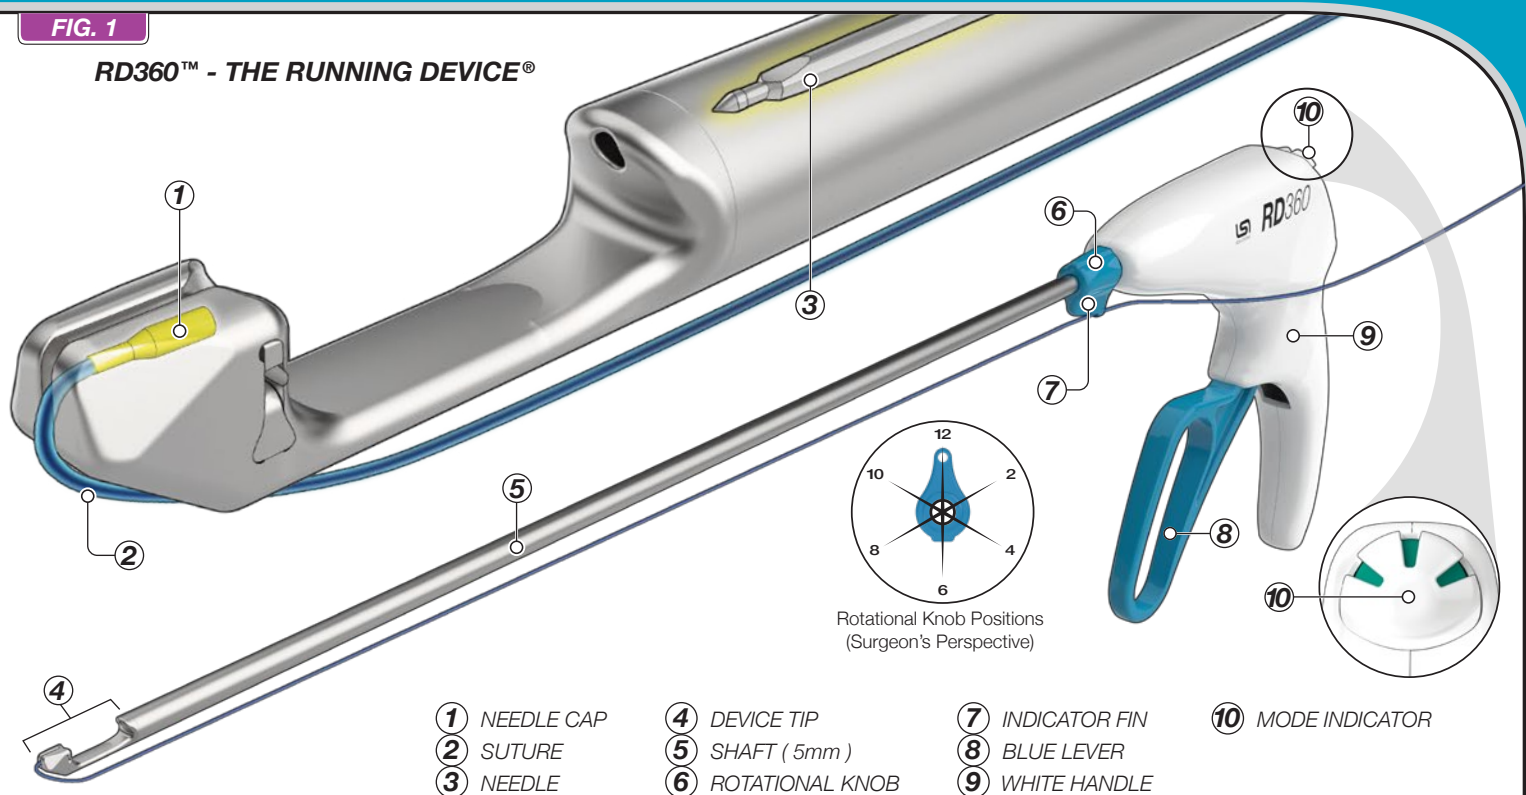

RD360™ - THE RUNNING DEVICE® DESCRIPTION

Each sterile package contains one RD360™ suturing device (FIG. 1). The RD360™ DEVICE is used for the placement of RD® QUICK LOAD® surgical suture. A short length of modified surgical stainless steel tubing, called a needle cap ①, is attached to the end of the suture ② in the RD® QUICK LOAD® unit. The RD360™ needle ③ is held retracted within the device tip ④ at the end of the 5mm diameter, 33cm length shaft ⑤. The shaft can be rotated 360° about its axis by turning the rotational knob ⑥, with the integrated indicator fin ⑦ corresponding to the non-sewing side of the device tip. The device blue lever ⑧ is attached to the white handle ⑨ and controls the device needle. Squeezing the lever causes the needle to advance, and releasing the lever causes the needle to retract. Fully squeezing and releasing the lever causes the device to alternate between its pickup and rearm modes. When the device is in pickup mode, a first full squeeze and release the lever advances the needle to engage with a needle cap loaded in the device tip and retracts the needle, now with needle cap and attached suture, back across the device tip. The next full squeeze and release of the lever will again advance the needle and needle cap with attached suture across the device tip, where a latch feature will retain the needle cap and suture as the needle retracts. Subsequently squeezing and releasing the lever will repeat this process and cycle the device between its pickup and rearm modes. The mode indicator ⑩ on the back of the white handle alternates between green (pickup mode) and white (rearm mode) to indicate which mode the device is in.


INDICATIONS

The RD360™ suturing device is indicated for use in the approximation of soft tissue and prosthetic materials.


LS SOLUTIONS®

FIG. 2

SUTURE PLACEMENT

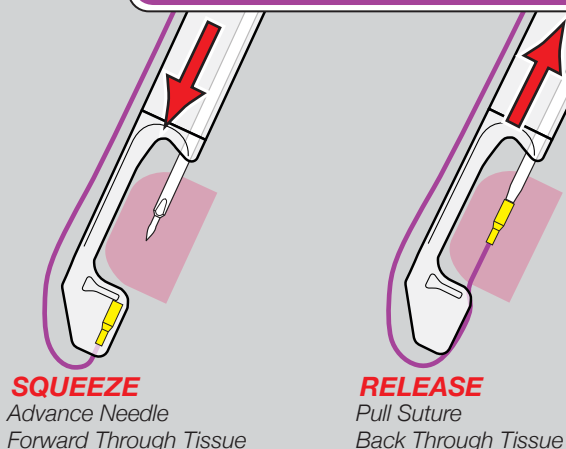

SUTURE REARM

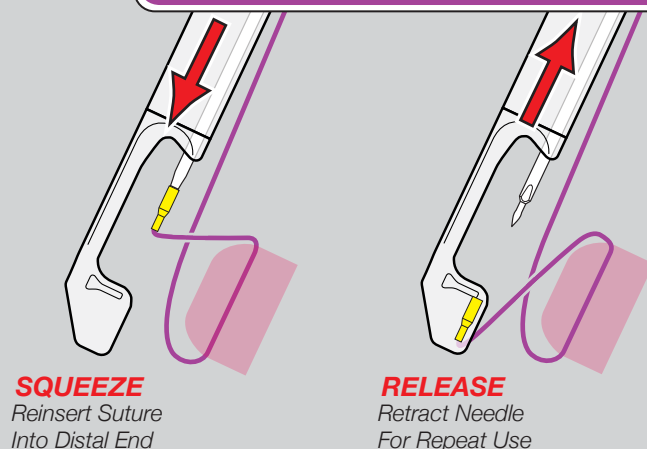


RD® QUICK LOAD® SUTURE

FIG. 3

RD® QUICK LOAD® SUTURE

- ① SUTURE TRAY
- ② SUTURE RELEASE FEATURE
- ③ NEEDLE CAP
- ④ SUTURE
- ⑤ SUTURE TUBE

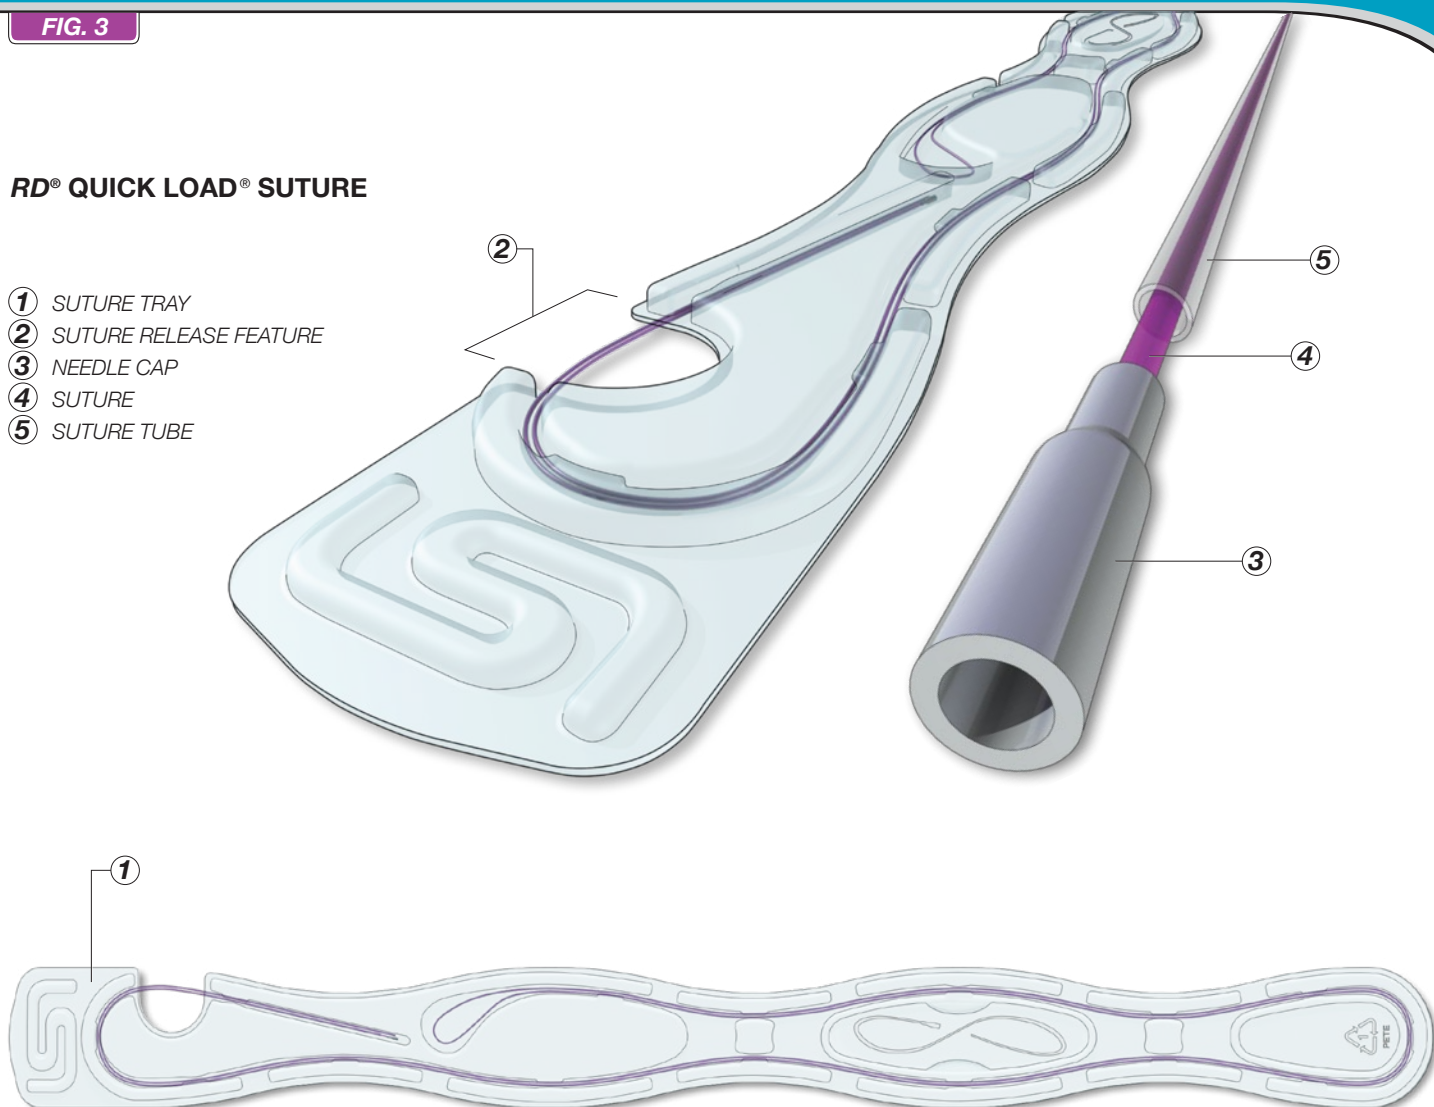

NOTE: RD® QUICK LOAD® Surgical Suture 2-0 Monoglide DUO not shown here.

L

DESCRIPTION

Each LSI SOLUTIONS® RD® QUICK LOAD® sterile suture is held in a customized tray (1) with suture release feature (2), designed to enable the rapid, easy and reliable loading of suture into RD®, RD180®, RD360™, and RD360 PLUS™ devices. RD® QUICK LOAD® suture products are available in excellent quality non-absorbable or absorbable suture materials in both braided and monofilament configurations (FIG. 6). A short length of modified surgical stainless steel tubing, called a needle cap (3), is attached to the end of the suture (4). The RD® QUICK LOAD® suture also includes a detachable clear suture tube (5) to keep the suture from tangling. Each sterile RD® QUICK LOAD® suture is individually packaged for single patient use.

INDICATIONS

RD® QUICK LOAD® suture is indicated for use in general soft tissue approximation, and/or ligation.

CAUTION:

To avoid accidental needle exposure, **DO NOT** squeeze lever during suture loading.

ACTIONS

To facilitate the placement of multiple stitches of the same suture (i.e., “running” or tying the suture) without needing to manually rearm each needle cap, the needle cap rearming mechanism of the *RD360™ DEVICE* enables the remote return and rearming of the needle cap back into the needle cap compartment. The operator presents an appropriate tissue structure into the gap of the metal jaw in the device tip of the *RD360™ DEVICE*. During suture placement, the blue lever is squeezed to advance the retracted needle from the shaft of the device through the tissue in the jaw and into the needle cap. The distal contoured end of the *RD360™ DEVICE* needle engages and captures the needle cap with its attached suture. Releasing the blue lever retracts the needle with attached needle cap and suture back through the tissue. For suture rearm, the distal tip is then moved away from any tissue structures to clear the jaw for needle cap resetting. The blue lever is again fully squeezed to advance the needle, needle cap and suture forward through the empty jaw toward the needle cap compartment at the most distal end of the device tip. Care must be taken to ensure the suture crimped to the distal end of the needle cap is oriented to permit the suture to freely pass through the suture track opening in the needle cap compartment. Jamming misoriented suture into the needle cap compartment can damage suture and device. With the blue lever fully squeezed and the needle with its attached needle cap and suture completely forward, the now rotated needle will permit the needle cap rearm latch to engage the face of the needle cap and cause its release from the needle. With the first tissue suture placement complete, the needle cap rearm into the needle cap compartment, and the blue lever back in its starting location, *RD360™ DEVICE* is ready for another tissue bite. This sequence can be repeated for up to 12 bites (or 12 complete functional cycles) with a single *RD® QUICK LOAD®* suture and with up to 12 *RD® QUICK LOAD®* sutures per device.

CONTRAINDICATIONS

- Minimally invasive surgical procedures should only be performed by physicians having adequate training and familiarity with endoscopic techniques. In addition, medical literature should be consulted relative to techniques, complications and hazards prior to the performance of minimally invasive procedures.
- RD360™ DEVICE* is not intended to be used with any suture other than *RD® QUICK LOAD®* suture.
- Do not use this suture under conditions in which excessive suture tension can lead to tissue damage. For example, do not use *RD® QUICK LOAD®* suture through an excessively narrow, restrictive or defective cannula access port, which could significantly impair easy and smooth passage of the suture or device.

WARNINGS

- Federal (U.S.A.) law restricts this device to sale, distribution and use by, or on the order of a physician.
- Do not resterilize.** The performance of *RD360™ DEVICE* after cleaning or other reprocessing has not been verified and is not supported by LSI SOLUTIONS®.
- Discard open, unused, expired or damaged devices or devices in damaged primary packaging.
- As with any foreign body, prolonged contact of any suture with salt solutions, such as those found in the urinary or biliary tracts, may result in calculus formation.
- Users should be familiar with surgical procedures and techniques involving suture before employing *RD360™ DEVICE* for wound closure, as the risk of wound dehiscence may vary with the site of application.
- Acceptable surgical practice must be followed with respect to drainage and closure of infected or contaminated wounds.
- Redundant, cut-away suture remnants, used needle caps, and *RD®* devices, along with packaging, must be inspected, handled and disposed of consistent with standard, accepted medical device disposal procedures.
- RD360™ DEVICE* is indicated for use in the approximation of soft tissue. Applications other than for soft tissue closure, or to anchor another device, can result in failure to pick up suture or in damage to the device making it unsuitable for continued use.
- Never drive the needle into suture, bone, dense ligamentous tissue, or other instruments.
- RD® QUICK LOAD®* suture is not for use in cardiovascular and neurological procedures.

PRECAUTIONS

- Check for hemostasis or leakage where appropriate.
- Minimally invasive instruments may vary in diameter from manufacturer to manufacturer. Before endoscopic instruments and accessories from different manufacturers are employed together in a procedure, verify compatibility and ensure electrical isolation or grounding are not compromised.
- Care must be taken when inserting this or any device through a cannula to avoid advancing the device incorrectly (e.g., too far or too quickly). Device insertion should be easy, smooth and controlled to minimize the risks of trauma to the patient or damage to the device.
- Always assure insufflation, camera position and device tip location are viewed under direct visualization before advancing the needle.
- Ensure obstructions do not interfere with the movement of the needle of *RD360™ DEVICE*.
- In handling *RD360™ DEVICE*, care should be taken to avoid jamming the suture into the needle cap compartment and damage to the needle.
- Avoid damage to the needle, suture or needle caps due to direct application of surgical instruments, like forceps, needle holders, clamps, etc.
- Adequate knot security requires accurate completion of accepted surgical techniques for constructing surgically tied knots or the use of the *TK® Ti-KNOT® DEVICE* and *TK® QUICK LOAD®* suture as warranted by surgical circumstances and the experience of the surgeon.
- Before loading *RD360™ DEVICE* with another *RD® QUICK LOAD®* suture, assure the remaining suture tail and needle cap from the previous load has been removed from the needle. Failure to appropriately remove used needle cap from the needle can result in damage to the device, including intracorporeal or extracorporeal fracturing off the tip of the needle, making it unsuitable for continued use.
- After each loading and re-loading of a new suture into this device, squeeze the blue lever to drive the needle forward into the new needle cap loaded into the needle cap compartment. If the needle cap is picked-up by the needle, then squeeze the lever again to rearm the needle cap and suture back behind the latch. If the needle rotation is oriented to rearm the needle cap, then the needle will retract back without the needle cap and suture attached. This “cycling” (FIG. 4, Step 5) of the needle helps ensure that the previous needle cap was properly removed, the new needle cap is installed properly, and the operator receives the device with its needle oriented to pick-up the needle cap on its first needle advancement. If the previous needle cap was not properly removed from the needle prior to reloading the device, the needle will not fully advance into the new needle cap in the needle cap compartment. Failure to avoid driving a needle with a needle cap into another needle cap can lead to the breaking off of the tip of the needle.
- Do not use *RD360™ DEVICE* to dissect or aggressively manipulate tissue structures.
- Verify that the needle cap is still retained within the needle cap compartment and the device has not been damaged or deformed before attempting to place a stitch.
- Do not manipulate the device at any time with the blue lever partially actuated. This may expose sharp surfaces that can cause trauma to the patient, the device operator or other staff, or damage the device.
- To avoid inadvertent suture damage, ensure the needle cap always enters the needle cap compartment with its suture oriented to freely pass through the needle cap compartment's suture track. Do not use damaged or expired suture.
- Ensure the advancing needle targets and enters the needle cap compartment. For example, during the suture placement, avoid using an extended needle to manipulate or lift tissue because such an action can cause the needle to deviate from its targeted course toward the needle cap compartment. A needle tip, not entering the needle cap compartment properly, can strike the distal tip of the device and lead to undesired outcomes, including needle tip fracture. For another example, during suture rearm, avoid applying tension to the suture from the needle cap on the needle. Tension on the suture can cause the needle to deviate off target and lead to the needle cap possibly striking the distal tip, which can cause needle tip fracture.
- Cautiously change modes while the *RD360™ DEVICE* is employed through a cannula. Failure to do so may result in improper tensioning of the suture.

ADVERSE REACTIONS


Adverse effects associated with the use of suture include wound dehiscence, failure of adequate wound support in closure sites where expansion, stretching or distension occur, enhanced bacterial infectivity, minimal acute inflammatory tissue reaction, localized irritation when skin sutures are left in place for greater than 7 days, calculi formation in urinary and biliary tracts when prolonged contact with salt solutions such as urine and bile occurs, and pain, edema and erythema.

LOADING SUTURE

CAUTION: To avoid accidental needle exposure, **DO NOT** squeeze lever during suture loading.


FIG. 4

1 **REMOVE** Suture And Suture Tube From Tray

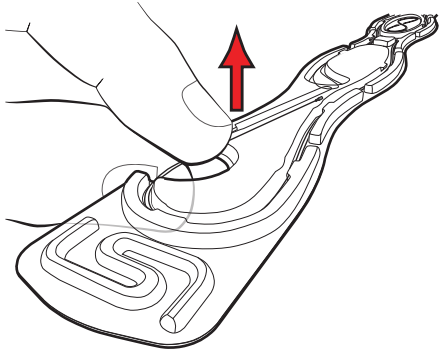


REMOVE suture and suture tube from tray by grasping suture tube at suture release feature and pulling suture tube completely out of tray.

2 **INSERT** Suture Into Suture Track




INSERT suture into the suture track as shown; may require pulling needle cap and suture further out of suture tube.

3 **PULL** Needle Cap Into Compartment




PULL suture to seat needle cap into needle cap compartment in the distal end of the device tip. It may help to guide the needle cap with a finger. Make sure needle cap is fully seated behind latch.

4 **REMOVE** Suture Tube



5 **FIRE & REARM**

Orient Suture As Shown, Squeeze And Release Lever To Ensure Suture Is Ready In Distal End Of Device Tip



FIRE & REARM to ensure suture is loaded properly. To avoid jamming the needle cap into the needle cap compartment, orient the suture directly away from the jaw as shown. While the device is in pickup mode (green indicator), squeeze the lever to advance the needle through the jaw and into the newly loaded needle cap. Release the lever to pick up and retract the needle cap with attached suture back on the needle into the shaft. This will cycle the device into rearm mode (white indicator). While continuing to orient the suture as shown, squeeze the lever to advance the needle, needle cap, and suture forward through the jaw to rearm the needle cap into its compartment. Release the lever again and retract back the now-empty needle, cycling the device back into pickup mode (green indicator) and leaving the needle cap and suture ready for patient use.


UNLOADING SUTURE

UNLOADING NEEDLE CAP AND REMAINING SUTURE FROM RD® DEVICE

The Auto-release Technique, as illustrated below (FIG. 5) is an easy method for removal of used needle caps from the needle prior to reloading a suturing device. This technique automatically removes the suture and needle cap from the needle by simply pulling the lever fully forward.

FIG. 5

AUTO-RELEASE Technique *Retract Suture Back. Pull Lever Fully Forward. Remove Suture With Needle Cap.*

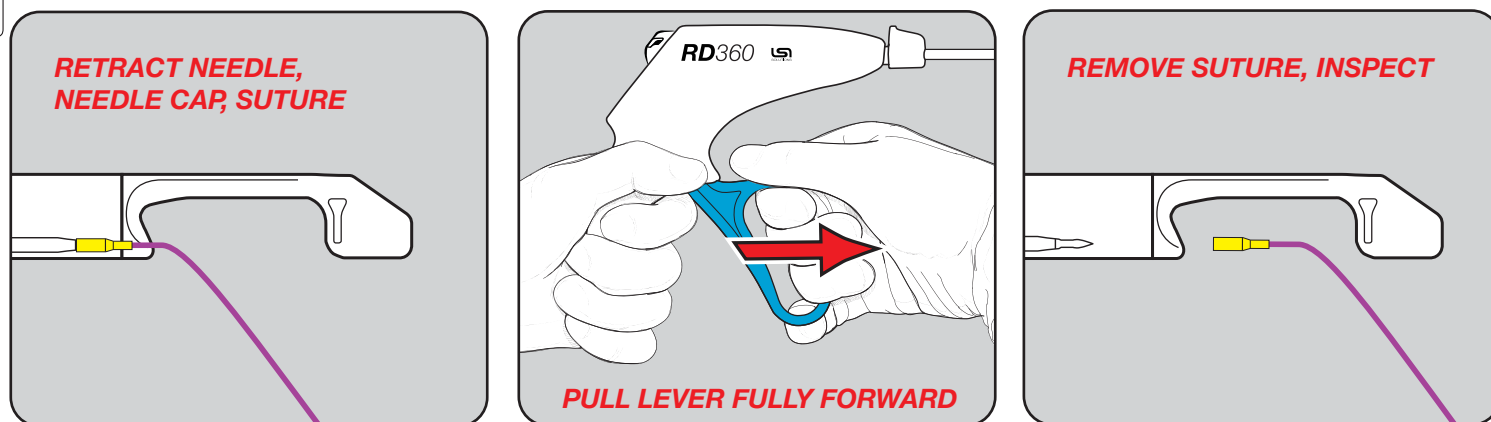




This unloading technique requires that the needle with its engaged needle cap and suture is retracted into the distal end of the device shaft and that the device is in rearm mode (white on the mode indicator). If the needle cap and attached suture are not engaged with the needle, squeeze and release the blue lever to pick up and retract the needle cap and attached suture. Once the needle cap, suture, and needle are retracted into the shaft and the device is in rearm mode, pull the lever fully forward to automatically remove the needle cap and suture from the needle. Inspect and discard the used needle cap and suture.

FIG. 6 PRODUCT ORDERING

SUPPLIED: STERILE

	REORDER	PRODUCT	DESCRIPTION
 x 6	REF 021000	RD360™ DEVICE , (33cm length)	Box of 6 Kits (1 Device per Kit)
 x 12	REF 020979	RD® QUICK LOAD® SURGICAL SUTURE 2-0 Polyester, Non-Absorbable, 53", Green, Braided, 1 Needle Cap	Box of 12 Sutures (1 Suture per Pouch)
 x 12	REF 021010	RD® QUICK LOAD® SURGICAL SUTURE 0 Polyester, Non-Absorbable, 53", Green, Braided, 1 Needle Cap	Box of 12 Sutures (1 Suture per Pouch)
 x 12	REF 020989	RD® QUICK LOAD® SURGICAL SUTURE 2-0 Polypropylene, Non-Absorbable, 53", Blue, Monofilament, 1 Needle Cap	Box of 12 Sutures (1 Suture per Pouch)
 x 12	REF 021025	RD® QUICK LOAD® SURGICAL SUTURE 2-0 Strongorb®, Absorbable, 53", Violet, Braided, 1 Needle Cap	Box of 12 Sutures (1 Suture per Pouch)
 x 12	REF 021030	RD® QUICK LOAD® SURGICAL SUTURE 2-0 Monoglide®, Absorbable, 53", Purple, Monofilament, 1 Needle Cap	Box of 12 Sutures (1 Suture per Pouch)
 x 12	REF 021506	RD® QUICK LOAD® SURGICAL SUTURE 0 Monoglide®, Absorbable, 53", Purple, Monofilament, 1 Needle Cap	Box of 12 Sutures (1 Suture per Pouch)
 x 12	REF 023387	RD® QUICK LOAD® SURGICAL SUTURE 2-0 Monoglide® DUO, Absorbable, 53", Purple, Monofilament, 2 Needle Caps	Box of 12 Sutures (1 Suture per Pouch)

RD360™ DEVICE TECHNIQUE PEARLS

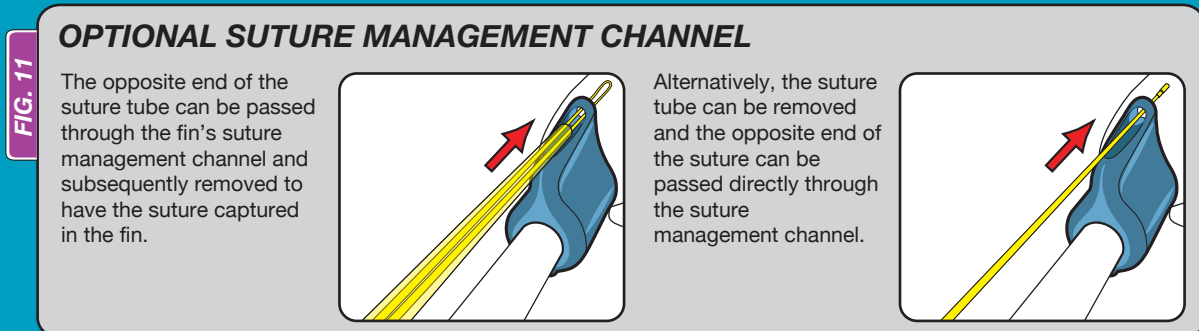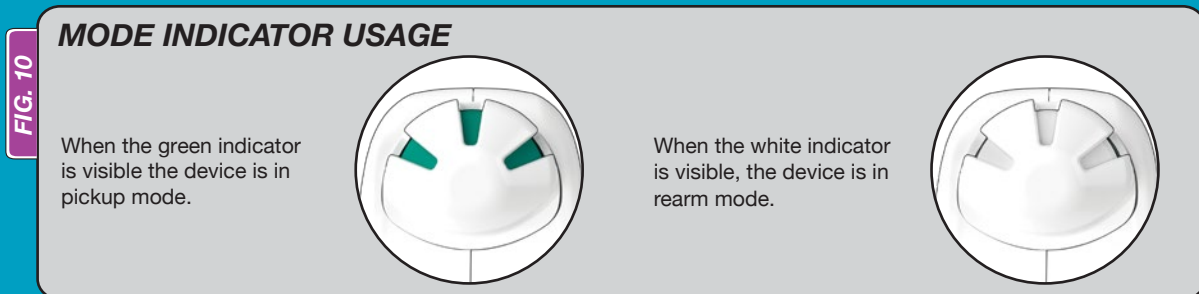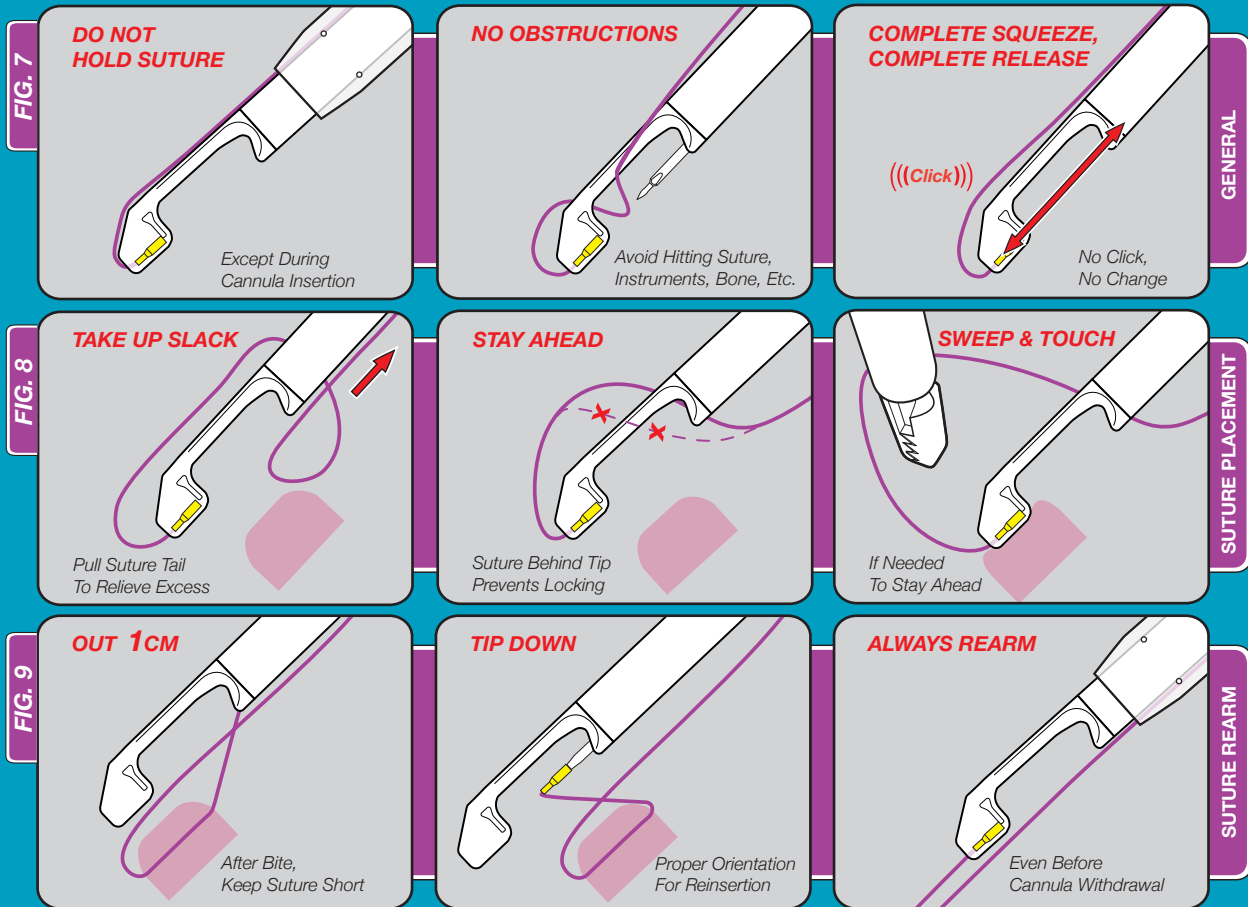

LSI SOLUTIONS®

Patents: www.lsisolutions.com/patents

The LSI logo, LSI SOLUTIONS, RD, The Running Device, RD360, RD360 PLUS, StrongSorb, MonoGlide, TK, Ti-Knot, Quick Load, and Perfect Performance Policy are trademarks and registered trademarks of LSI SOLUTIONS®.



STERILE EO

Rx Only



MD

Symbol Glossary: www.lsisolutions.com/symbols



LSI SOLUTIONS®
7796 Victor-Mendon Road
Victor, New York 14564 U.S.A.
Phone: 585.869.6600
Customer Service: 866.575.3493
Technical Support: 866.428.9092
Fax: 585.742.8086
www.lsisolutions.com

MADE IN THE USA

This Product Comes
with our LSI SOLUTIONS®
Perfect Performance Policy®
Call us at 866.575.3493 any time.