
A large green circle is positioned in the lower-left quadrant of the page. It is surrounded by a cloud of small green dots of varying sizes, which appear to be radiating from the circle's edge.

Designed for  
Precision  
and Performance

# Supernova

Revascularization Device



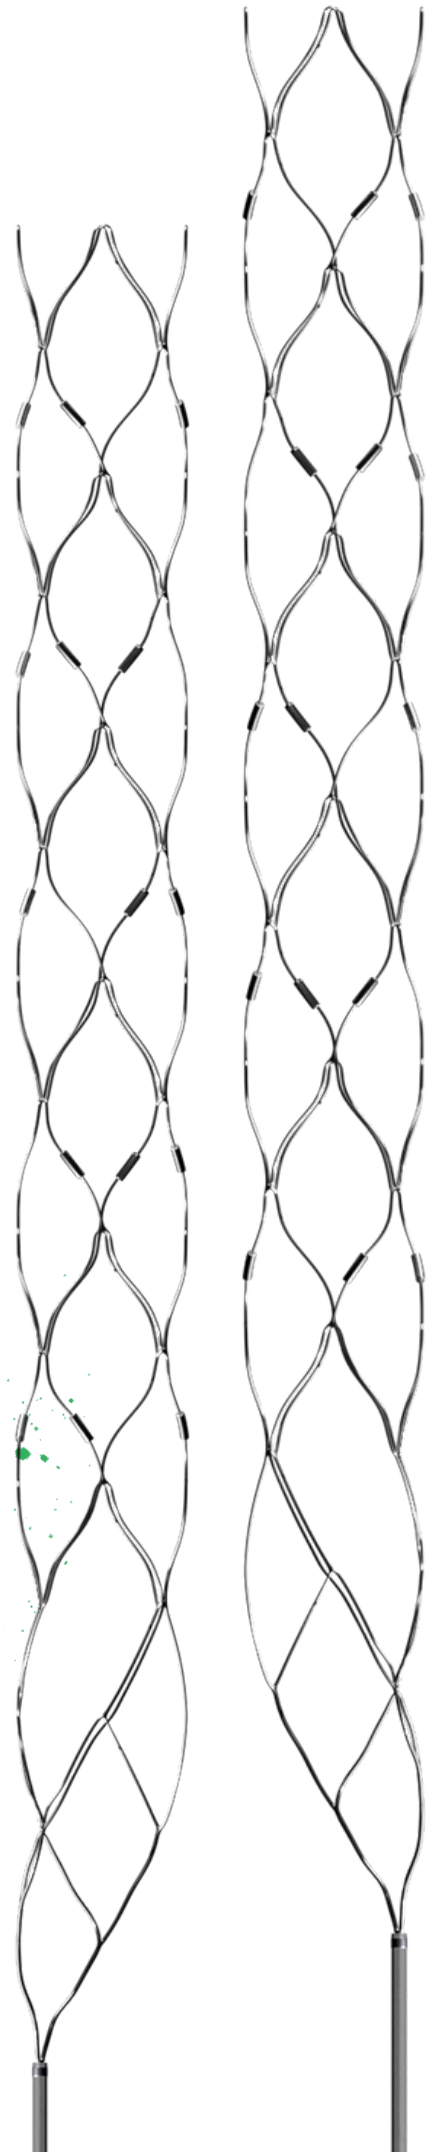

## Advanced Clot Capture Technology



### Spiral Fusiform Technology

Ensures superior engagement and retrieval of both red and hard fibrin-rich (white) clots.



### Optimized Radial Force

Provides effective deployment and retrieval, maintaining consistent performance.



### Radiopaque Markers

Ensures visual confirmation under fluoroscopy for accurate positioning.

# 95%

mTICI  $\geq$ 2B

Recanalization Success Rate

# 63%

First Pass Success Rate

To Achieve Effective Reperfusion



### Dynamic Strut Activity

Engineered for optimal flexibility and control during deployment and retrieval.

### Supernova Revascularization Device Specifications

Model	Working Length	Stent Diameter	Vessel Diameter Range	Radiopaque Markers	Delivery Catheter ID
GRVY-004-043	136cm	4mm	1.5mm - 4.0mm	12	0.021"
GRVY-006-047	125cm	6mm	2.0mm - 5.5mm	15	0.021"



### Optimize Your Stroke Intervention

Join the leading experts in stroke care and enhance your clinical practice with the Supernova Revascularization Device. Experience the unmatched performance and reliability that Supernova offers in the most challenging clinical scenarios.